MIDMARK

Installation/Operation Instructions

9A267001/002 INSTRUMENT TRAY

KIT COMPONENTS

Part Number	Description	Qty.
9A267001	Instrument Tray Assy. Double Arm	1
9A267002	Instrument Tray Assy. Single Arm	1
• 016-0289-00	Tray, Instrument	1
• 030-1215-00	Arm Extension Weldment	1 or 2
• 052-0338-00	Rod, Mounting	1
• 030-1214-00	Rail Mount Weldment	1
• 520-0055-10	T-handle	3 or 4
• 516-0258-00	Thumb Screw	1
• 003-0936-00	I / O Instructions	1

REQUIRED TOOLS

None

INTRODUCTION

To hold instruments for an examination or general procedure. Used in conjunction with 9A272 Base Rail.

WARNING

Must be mounted on base rail of exam table. Must be removed or rotated clear of moving parts before positioning table. Always support Instrument Tray when changing positions. Assure all positions are solidly locked to prevent movement during procedure.

Maximum Weight Limitations (centered on tray):

Double Arm Tray (9A267001)
Models 411 and 419: 15 lbs (6.8 kg)
Models 119, 311, and 319: 5 lbs (2.3 kg)

Single Arm Tray (9A267002)
Models 411 and 419: 30 lbs (13.6 kg)
Models 119, 311, and 319: 10 lbs (4.6 kg)

Do not use more than one Instrument Tray simultaneously on same side of table.

INSTALLATION (1)

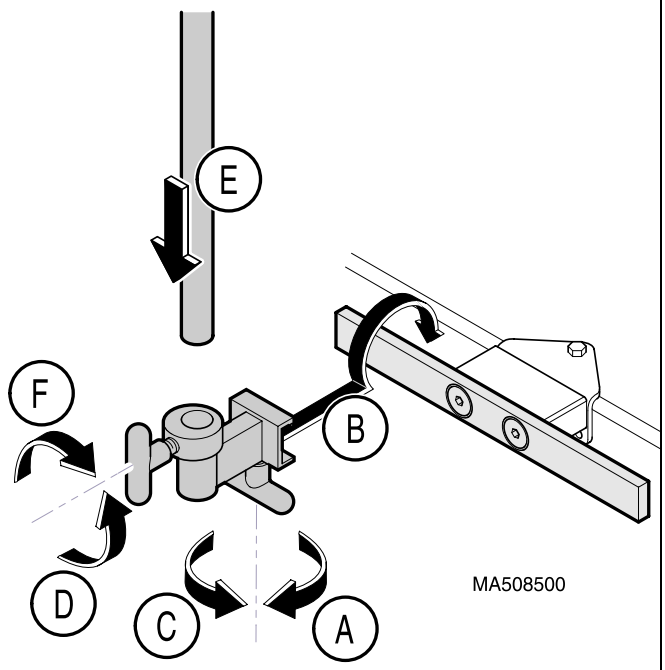

EQUIPMENT ALERT

Place table in desired position before mounting 9A267 Instrument Tray. Do not operate table after Tray has been installed to prevent damage to table or Tray.

A. Loosen handle on Rail Mount Weldment.

WARNING

T-handle that secures Rail Mount must be positioned below Base Rail so lip on Rail Mount hooks over top of Base Rail.

B. Hook Rail Mount over or slide it onto Base Rail.
C. Tighten handle.
D. Loosen handle.
E. Insert Mounting Rod.
F. Tighten handle.

© Midmark Corporation - 1999

INSTALLATION (2)

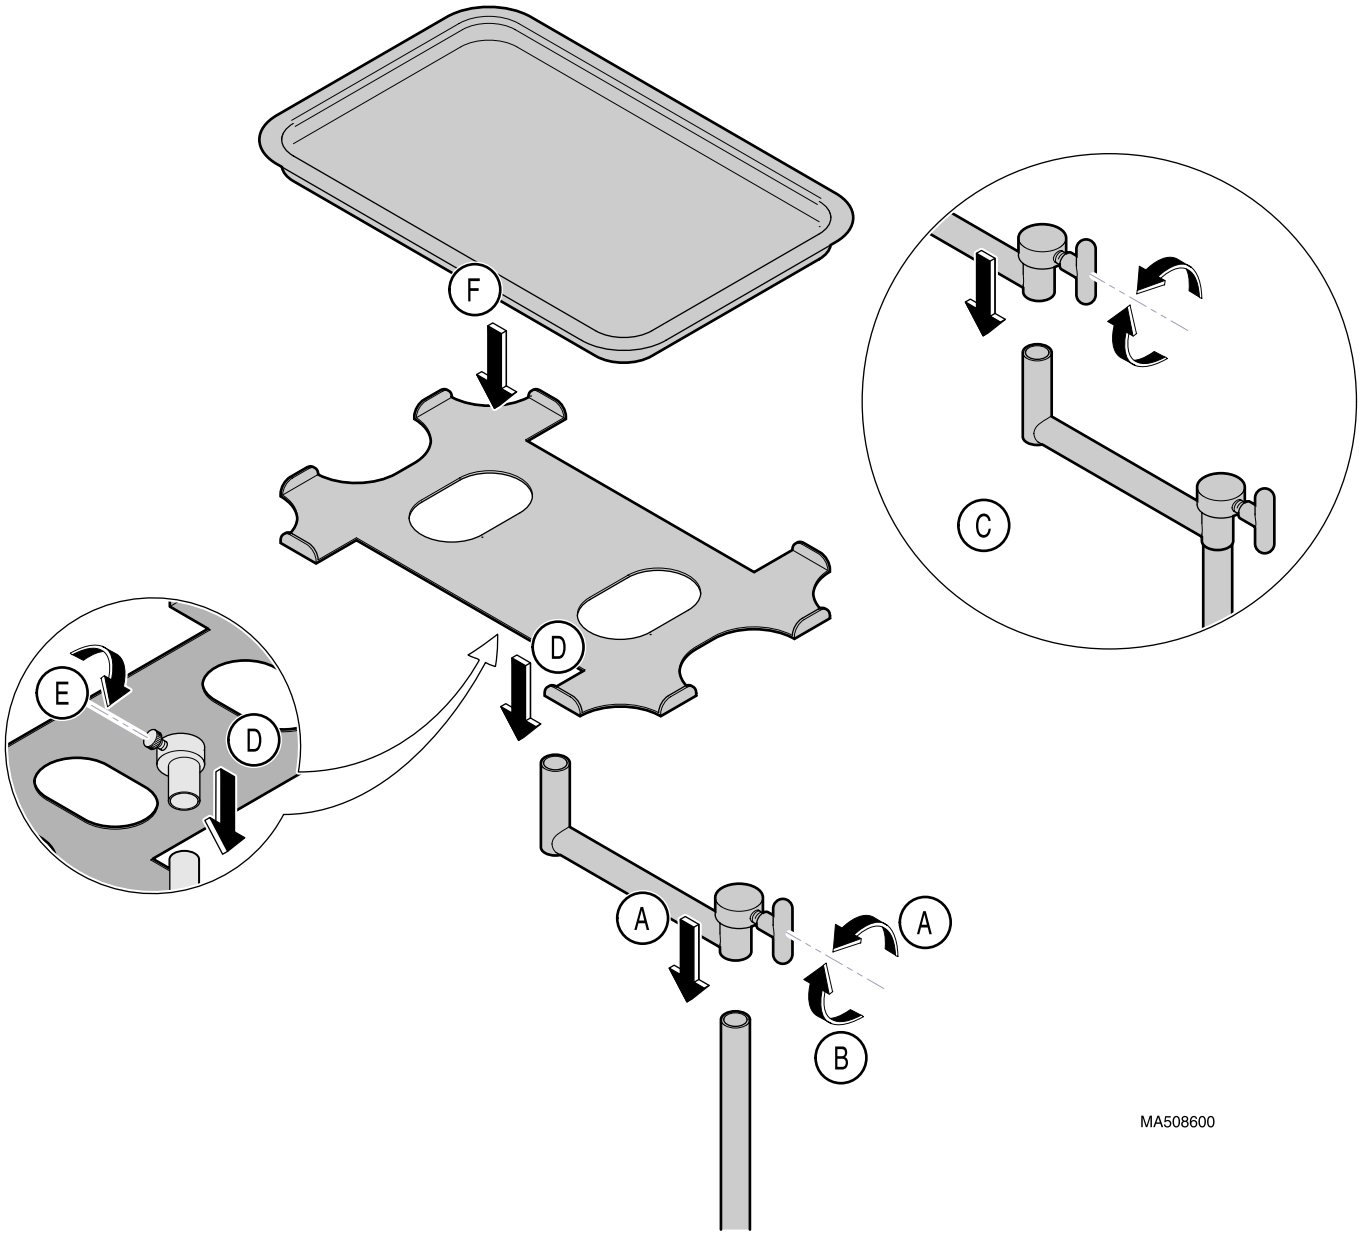

WARNING

Assure Arm Extensions are <u>completely engaged</u> when mounting before tightening T-handles. Failure to comply could result in disengagement during procedure and personal injury.

- **A.** Loosen handle on Arm Extension and insert onto Mounting Rod.
- **B.** Tighten handle.
- **C.** When applicable, mount second Arm Extension to mounting tube of first arm extension
- **D.** Install Tray Mount Weldment onto mounting tube of Arm Extension.
- **E.** Tighten thumb screw.
- **F.** Place Tray in position.

NOTE

To reposition Tray, while <u>supporting</u> assembly, loosen appropriate handle(s), reposition, then retighten handles.

MIDMARK®

Midmark Corporation, Versailles, Ohio 45380 U.S.A.
(937) 526-3662 FAX (937) 526-5542

003-1026-00 Rev. C (1/01)

© Midmark Corporation - 1999